



SPECIFICATION FOR APPROVAL

MODEL NUMBER	HDP05-MD05010U
PART NUMBER	HDP05-MD-0005
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK, USB, with EU ,AU ,UK adapter
CUSTOMER / PROJECT CODE	MED-01
REVISION	A0
DATE	March 11, 2022

CUSTOMER APPROVAL	DATE
SEACOMP ENGINEERING APPROVAL	DATE

HDP Power – a SEACOMP company
2546 Gateway Road
Carlsbad, California 92009

Tel: 1.760.438.9600
Email: sales@seacomp.com
Website: www.hdp-power.com



MODEL NUMBER	HDP05-MD05010U	PAGE	1 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

Contents

Contents	1
Revision History	2
1 Scope	3
2 Quality Requirements	3
2.1 Product Specific Quality Requirements	3
2.2 General Quality Requirements	5
3 Electrical Characteristics	7
3.1 Input	7
3.2 Output	7
3.3 Connector	8
4 Cosmetic	9
4.1 Surface Definitions	9
4.2 Inspection Conditions	9
4.3 Cosmetic Defect Definitions	10
4.4 Size / Weight	12
4.5 Assembly Drawing	13
5 Electromagnetic Compatibility	17
6 Labeling	18
6.1 Labeling the Device	18
6.2 Label Drawing	18
7 Packaging	19
7.1 Drawing	19
7.2 Packaging Test	22
8 Warranty	22



Revision History

[illegible]

MODEL NUMBER	HDP05-MD05010U	PAGE	3 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

1 Scope

The device is a 5-watt AC to DC adapter designed to provide a constant power source for electrical products. This adapter is certified for both medical and informational technology equipment (ITE) applications.

2 Quality Requirements

2.1 Product Specific Quality Requirements

2.1.1 Mechanical / Electrical Requirements

2.1.1.1 Paint and Print Test

In accordance with EN 60068-2-70

The printings have to withstand the testing procedures without any restrictions.

Test liquid	Mineral oils (example: Baby oil)
Wiping cycles	1,000
Contact pressure	1N $\pm$ 0.2N

2.1.1.2 Mechanical and Electrical Reliability

All electrical contacts and mechanically moving parts have to withstand a stress test of at least 3,000 simulated connecting cycles without any damage. After the test, the device must have 100% functionality. Connectors must comply with the manufacturer's requirements or relevant standards at minimum.

2.1.1.3 Cable Tension and Flex

All cable joints and strain relief points have to pass the following:

Static load:	5Kg / 1 min at 0 degree and at 90 degree angles
Flex test:	+/- 60 degree bending angle 250gm at 20cycle / minute with a minimum speed of 1000 cycles.

2.1.1.4 Drop Test

This test requires the device to be dropped from a height of 1 meter onto a concrete floor. The drop should cover all surfaces including the 2 edges and all 4 corners. After the test, the device should have 100% functionality. There should not be any cracks, breaks or damage to any surface or have any loose internal components. Additionally, the ultrasonic weld joint should still be intact with minimum 80% coverage.

2.1.1.5 Enclosure Crush Test

This test applies a uniformly distributed weight of 250 Newtons on all surfaces for 5 seconds per surface. There should be no physical damage or effect on the products performance (i.e. operating folding AC blade, easy insertion of international adapters, snug USB connector fit).

2.1.1.6 Cable Burn Test (to be tested by safety lab)

In accordance with DIN 75200

Burn down speed	max. 50 mm/min
-----------------	----------------

UL rated cable with UL file is an acceptable replacement for this test. Cable to be VW-1 rated.

MODEL NUMBER	HDP05-MD05010U	PAGE	4 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

2.1.2 Climate Requirements

2.1.2.1 Temperature Range

Full Functionality	0°C up to +50°C
Storage Temperature	-20°C up to +85°C

2.1.2.2 Thermal Shock (operational)

Low Temperature	0°C (AC/DC)
High Temperature	50°C (AC/DC)
T / t	15°C/min
Cycle Duration	1 hour
Number of Cycles	10
Mode of Operation	Minimum 75% full load
Requirement	100% functionality after test, without any damages or physical change

2.1.2.3 Thermal Shock (non-operating)

Low Temperature	-20°C
High Temperature	+85°C
T / t	15°C/min
Cycle Duration	1 hour
Number of Cycles	10
Mode of Operation	Switched off
Requirement	100% functionality after test, without any damages or physical change

2.1.2.4 Thermal Aging

Temperature	-20°C and +85°C
Duration	96 hours at each temperature
Mode of Operation	Power off
Requirement	100% functionality after test, without any damages or physical change

2.1.2.5 Humidity (non-condensing)

Temperature	+45°C
Humidity	95%
Duration	96 hours
Mode of Operation	Power up no load
Requirement	100% functionality after test, without any damages or physical change

2.1.2.6 Humidity (condensing)

Upper Temperature	+45°C
Lower Temperature	+25°C
Humidity	95%
Test Cycle	5°C / max ramp rate
Duration	96 hours
Number of cycles	6
Mode of Operation	Power up no load
Requirement	100% functionality after test, without any damages or physical change

MODEL NUMBER	HDP05-MD05010U	PAGE	5 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

2.1.2.7 Salt Spray

Follow ASTM B117 standard with the possible exceptions listed below.

Temperature	35°C + 1.1 / - 1.7°C
Salt Solution	5%+/-1 Salt solution (NaCl) in Distilled or D1193 Type IV water
PH	6.5 - 7.2
Fog Rate	1m - 2 mL / hr / 80sq.cm
Duration	24 hours

2.2 General Quality Requirements

2.2.1 Product Related Requirements

2.2.1.1 General Appearance

Follows cosmetic requirements listed in Section 4 of this specification.

2.2.1.2 Emissions

The device must not produce any nuisance or unhealthy smell. A certificate must be made available proving the use of harmless materials.

2.2.1.3 Product Safety

The product has to comply with the relevant requirements listed in IEC 60950, IEC62368 (ITE) and IEC 60601 (medical).

Normal usage of the product must not result in any danger. In particular, any broken component parts, including electric components, may not result in any risk or danger of injury to the user. This is to be proven by a risk analysis during the product's development phase. Any potential hazard has to be indicated clearly in the user manual.

During normal use at an ambient temperature of 25°C, the housing (made of synthetic material) may warm up by 50K. Therefore, the maximum temperature of the parts could be as high as 75°C.

Individual "Hot Spots" (maximum size of 2 cm²) is acceptable if they are not located in the grip area. A warm up by 60K is acceptable in these "Hot Spots." Therefore, the maximum temperature of these parts could be 85°C.

For both normal use and "Hot Spot" instances, the housing must not exceed the maximum temperature of the applied synthetic.

When using tantalum capacitors, the effects of a potential explosion must be reduced to prevent any hazard to the user's health.

Protective actions against confusing the poles of the electric connectors have to be taken for any internal parts or connectors with specific polarity.

Transportation, storage, and operation of the adapter must not create any hazard, personal injury or any material damage. This is guaranteed through the controllable quality of workmanship and material used.

It must be guaranteed that after contact with natural oils, the housing material's performance does not result in any dangerous situations to the customer.

MODEL NUMBER	HDP05-MD05010U	PAGE	6 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

2.2.1.4 Recycling and Environmental Compatibility

Must comply with RoHS and REACH.

Quality Level, (AQL)

In accordance with DIN ISO 2859 Part 1

General test-level	II
Critical defects	AQL 0
Major defects	AQL 0.4
Minor defects	AQL 0.65

2.2.2 Supplier Related Requirements

2.2.2.1 Demonstration of Quality

The supplier is obliged to maintain a quality assurance system which covers R&D and production specific items. This system must meet the requirements of ISO 9000-2008. A quality assurance plan (QA plan) is required for a project-specific proof of quality-assuring measures. The plan should be made available and presented upon request.

For the development phase, the QA plan needs to define milestones as proof of the reliability prognoses. The development results and the release by the customer need to also be included in this plan.

For the production phase, the QA plan has to focus on the detailed verification of all the planned QA steps from component procurement to delivery. Any acceptance or error criteria to be applied to the QA plan must meet the process capability index as defined in this specification.

2.2.2.2 Process Assurance

The quality capability has to be proven by a process capability of $C_{pk} > 1.33$ and must be documented by a continuous monitoring of the production process. Parameters relevant for this process capability will be marked separately in the product's construction documents.

2.2.2.3 Reliability

The probability of failure and the return of devices for repair must be less than 1% per year. The failure rates have to be predicted using MTBF calculations. The MTBF calculations have to be proven and available to the customer upon request.

A minimum of 100k MTBF must be achieved under nominal load and 25°C ambient temperature.

MODEL NUMBER	HDP05-MD05010U	PAGE	7 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

3 Electrical Characteristics

3.1 Input

- 3.1.1 Input Voltage Nominal: 120/220 VAC
- 3.1.2 Input Voltage Range: 90 ~ 264 VAC
- 3.1.3 Input Frequency Range: 50 / 60Hz (47 ~ 63 Hz)
- 3.1.4 Inrush Current: 50A peak at 240AC input < 200us
- 3.1.5 Maximum Input Current: 0.15A measured at 5 Watts
Vin = 100VAC & 1A load
- 3.1.6 Efficiency: CEC-VI
- 3.1.7 Turn-on Time: < 60ms
- 3.1.8 Input Fuse: 2A / 250VAC standard blow
- 3.1.9 AC Input Receptacle Type: Folding US AC blades
- 3.1.10 Isolation Voltage: Meet IEC 60950, IEC62368, IEC 60601
- 3.1.11 AC Leakage Current: .15mA measured 264V & 63Hz
- 3.1.12 Dielectric withstands Voltage: 3000VAC 60sec or 4242VDC 60 sec with no breakdown;
Earth leakage at 110% of rated voltage should be < 10mA
- 3.1.13 Input Power (No Load): < 0.1W

3.2 Output

- 3.2.1 DC Output: 5.00 VDC
- 3.2.2 Output Current: 1A
- 3.2.3 Load Regulation: 5% VDC
- 3.2.4 Ripple and Noise: 100mVp-p
- 3.2.5 Turn-on Overshoot: < 10%
- 3.2.6 Over-current Protection: < 30% of Imax
- 3.2.7 Short Circuit Protection: Protected for continuous short circuit
- 3.2.8 Reset After Shutdown: Yes
- 3.2.9 Thermal Stability Time: 30 min
- 3.2.10 Peak Load Duration: Indefinite (OCP will prevent overload)

MODEL NUMBER	HDP05-MD05010U	PAGE	8 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

3.3 Connector

Option A: USB-A connector with Bridged (D+ and D- shorted) or MFI configuration connection.



4 Pin Male "A" Connector on the cable



4 Pin Female "A" Connector on the computer



4 Pin "B" Male Connector on cable



4 Pin "B" Female Connector on computer

5V / 1A MFI configuration		
ID Pin	D-	D+
Spec (V)	2.68	2
Tolerance (V)	2.44-2.89	1.84-2.16
Non MFI Bridged version		
ID PIN	D/D shorted	

Pin	Name	Description	Color
1	VCC	+5 VDC	Red
2	D-	Data -	White
3	D+	Data +	Green
4	GND	Ground	Black



MODEL NUMBER	HDP05-MD05010U	PAGE	9 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

4 Cosmetic

4.1 Surface Definitions

Level A is the primary surface. For example, the front face of the adapter.

Level B is a secondary surface that may be viewed periodically by the end user, but is not in direct view during normal use. For example, the Cable (AC and DC), the sides of the housing, and the back of the housing.

Level C surfaces are not visible by the end user. For example, the inaccessible inside surfaces of the product.

4.2 Inspection Conditions

4.2.1 Inspection Method: Light source: Cool white fluorescent lamp 750 – 1000Lux

4.2.2 Viewing Distance: 30cm

4.2.3 Viewing Angle: 0 – 90 Degrees

4.2.4 Part Rotation Angle During Inspection:

Vertical Rotation Angle 180 Degrees

Horizontal Rotation Angle 360 Degrees

4.2.5 Viewing Time:

5 seconds total for all surfaces

MODEL NUMBER	HDP05-MD05010U	PAGE	10 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

4.3 Cosmetic Defect Definitions

Defect	Level A	Level B	Level C
Scratches, Dents, and Burrs (see Note 1)	Single defect not exceeding total surface area 5.50 mm ²	Two defects not exceeding total surface area 11 mm ²	Accept if it does not affect fit or function
Hairline Scratches, Gate Blush/Trim, Stress	Use 25% Contrast Standard to accept or reject for visible hairline scratches with depth of < 0.1 mm (total surface area not to exceed limits set in surface scratch below)		
Surface Scratches, Scuffs (see Note 1)	Single defect not exceeding total surface area of 5.7 mm ²	Two defects not exceeding total surface area 25 mm ²	Accept if it does not affect fit or function
Chips, Nicks, Cracks or Broken Features	Not Allowed		
Flash, Burrs, Sink Marks (see Note 2)	Not Allowed	Less than 0.5mm	Accept if it does not affect fit or function
Discoloration	Follow color samples		
Parting Lines	See diagram		
General Stains (not permanent)	Not allowed		
Rust	Not allowed		
Printing	No missing text or mistakes allowed. All letters should be visible. Refer to approved sample.		

Note 1:

Area called out in these fields are calculated based on limit samples. The values are calculated based on average area covered by the features.

Note 2:

DC over-mold flash marks have to be signed off on samples and provided as acceptable limits.

MODEL NUMBER	HDP05-MD05010U	PAGE	11 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

Parting Line

Translation: 1. production for all components shall not be started before confirmation by HDP engineer. 2. Dimensions marked as ① are HDP control dimensions (to be inspected by IQC). 3. Dimensions marked as ② are customer control dimensions (to be inspected by IQC). 4. Dimensions unmarked please refer to 3D CAD. 5. Material should comply with ROHS standard. 6. Maximum draft angle is 1° unless otherwise notified. 7. diameters unmarked in drawing are 0.2mm. 8. Material: _____ (weight: $\pm 5\%$). 9. Surface treatment: _____.		Third Angle Projection The sealing is the property of HDP corporation. Any reference or distribution by others is strictly prohibited and prohibited for the side use of the patented trademark. Any reference or distribution by others is strictly prohibited and prohibited for the side use of the patented trademark. Scale : 1:1 Unit : MM Version NO.: A0 Drawn By: 周英群 Checked By: 2015.05.26 Sample Tolling Official Issue		Tolerance Angular $\pm 0.25^\circ$ <table><thead><tr><th>Dimension</th><th>F</th><th>G</th><th>H</th><th>J</th></tr></thead><tbody><tr><td>0-8</td><td>± 0.09</td><td>± 0.17</td><td>± 0.1</td><td>± 0.2</td></tr><tr><td>8-25</td><td>± 0.09</td><td>± 0.15</td><td>± 0.15</td><td>± 0.2</td></tr><tr><td>25-40</td><td>± 0.12</td><td>± 0.2</td><td>± 0.25</td><td>± 0.4</td></tr><tr><td>40-60</td><td>± 0.15</td><td>± 0.25</td><td>± 0.3</td><td>± 0.6</td></tr><tr><td>60-80</td><td>± 0.15</td><td>± 0.3</td><td>± 0.4</td><td>± 0.6</td></tr><tr><td>80-100</td><td>± 0.15</td><td>± 0.3</td><td>± 0.4</td><td>± 0.6</td></tr><tr><td>100-125</td><td>± 0.15</td><td>± 0.3</td><td>± 0.4</td><td>± 0.6</td></tr><tr><td>125-150</td><td>± 0.15</td><td>± 0.3</td><td>± 0.4</td><td>± 0.6</td></tr><tr><td>150-175</td><td>± 0.15</td><td>± 0.3</td><td>± 0.4</td><td>± 0.6</td></tr><tr><td>175-200</td><td>± 0.15</td><td>± 0.3</td><td>± 0.4</td><td>± 0.6</td></tr><tr><td>200-225</td><td>± 0.15</td><td>± 0.3</td><td>± 0.4</td><td>± 0.6</td></tr><tr><td>225-250</td><td>± 0.15</td><td>± 0.3</td><td>± 0.4</td><td>± 0.6</td></tr><tr><td>250+</td><td>± 0.15</td><td>± 0.3</td><td>± 0.4</td><td>± 0.6</td></tr></tbody></table>		Dimension	F	G	H	J	0-8	± 0.09	± 0.17	± 0.1	± 0.2	8-25	± 0.09	± 0.15	± 0.15	± 0.2	25-40	± 0.12	± 0.2	± 0.25	± 0.4	40-60	± 0.15	± 0.25	± 0.3	± 0.6	60-80	± 0.15	± 0.3	± 0.4	± 0.6	80-100	± 0.15	± 0.3	± 0.4	± 0.6	100-125	± 0.15	± 0.3	± 0.4	± 0.6	125-150	± 0.15	± 0.3	± 0.4	± 0.6	150-175	± 0.15	± 0.3	± 0.4	± 0.6	175-200	± 0.15	± 0.3	± 0.4	± 0.6	200-225	± 0.15	± 0.3	± 0.4	± 0.6	225-250	± 0.15	± 0.3	± 0.4	± 0.6	250+	± 0.15	± 0.3	± 0.4	± 0.6	Cons. Model NO. 110P HDP Model NO. 110P Part NO. 110P-01 Part NO. Part Name. 英1线图示 PMED004	
Dimension	F	G	H	J																																																																									
0-8	± 0.09	± 0.17	± 0.1	± 0.2																																																																									
8-25	± 0.09	± 0.15	± 0.15	± 0.2																																																																									
25-40	± 0.12	± 0.2	± 0.25	± 0.4																																																																									
40-60	± 0.15	± 0.25	± 0.3	± 0.6																																																																									
60-80	± 0.15	± 0.3	± 0.4	± 0.6																																																																									
80-100	± 0.15	± 0.3	± 0.4	± 0.6																																																																									
100-125	± 0.15	± 0.3	± 0.4	± 0.6																																																																									
125-150	± 0.15	± 0.3	± 0.4	± 0.6																																																																									
150-175	± 0.15	± 0.3	± 0.4	± 0.6																																																																									
175-200	± 0.15	± 0.3	± 0.4	± 0.6																																																																									
200-225	± 0.15	± 0.3	± 0.4	± 0.6																																																																									
225-250	± 0.15	± 0.3	± 0.4	± 0.6																																																																									
250+	± 0.15	± 0.3	± 0.4	± 0.6																																																																									

0.5 MAX

A

B

Tolerance Gap from side A to B 0.4mm

MODEL NUMBER	HDP05-MD05010U	PAGE	12 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022





4.4 Size / Weight

Product size should be 41.75W X 60.25L X 18.45H mm. Product weight is 40gm (weight does not include international adapters).

Transition:

1. production for all components shall not be started before confirmation by HDP engineer.
2. Dimensions marked as ① are HDP control dimensions (to be inspected by IQC).
3. Dimensions marked as ② are customer control dimensions (to be inspected by IQC).
4. Dimensions unmarked please refer to 3D CAD.
5. Material should comply with ROHS standard.
6. Maximum draft angle is 1° unless otherwise notified.
7. diameters unmarked in drawing are 0.2mm.
8. Material: _____ (weight: $\pm 5\%$).
9. Surface treatment: _____.
10. Angular measurements: (+) counter-clockwise direction.

REV.	DESCRIPTION	BY	DATE	ECN NO.
①	初版发行	YP.Zhou	2019.06.26	
②	增加IEC要求	YP.Zhou	2019.06.10	
③				

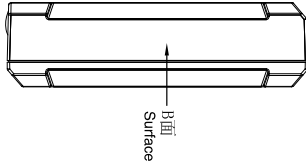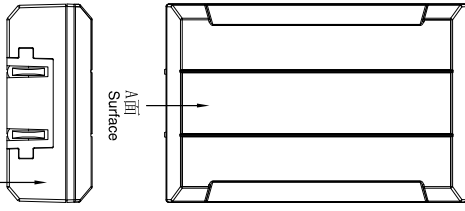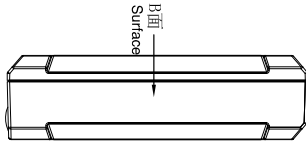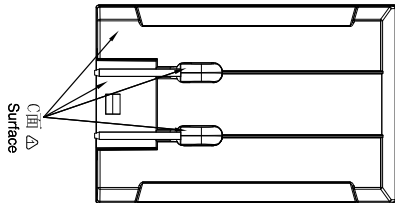HDP
a seacomp company

Third Angle Projection

Version NO.: 1
Scale: 1:1
Unit: MM
Drawn By: 周英鹏
Checked By: _____
Approved By: _____

Dimension F G H J
0-8 0.05 0.1 0.1 0.2
8-25 0.05 0.1 0.1 0.2
25-40 0.1 0.2 0.2 0.2
40-60 0.1 0.2 0.2 0.2
60-250 0.1 0.2 0.2 0.2
250-800 0.1 0.2 0.2 0.2
800-2500 0.1 0.2 0.2 0.2

Part No. _____
Part Name: 充电器面指示
FAB0004


This drawing is the property of HDP company. It is to be used for the production of the product only. It is not to be distributed to other parties without the written permission of HDP company.

Dimension F G H J
0-8 0.05 0.1 0.1 0.2
8-25 0.05 0.1 0.1 0.2
25-40 0.1 0.2 0.2 0.2
40-60 0.1 0.2 0.2 0.2
60-250 0.1 0.2 0.2 0.2
250-800 0.1 0.2 0.2 0.2
800-2500 0.1 0.2 0.2 0.2

Part No. _____
Part Name: 充电器面指示
FAB0004


MODEL NUMBER	HDP05-MD05010U	PAGE	13 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

4.5 Assembly Drawing

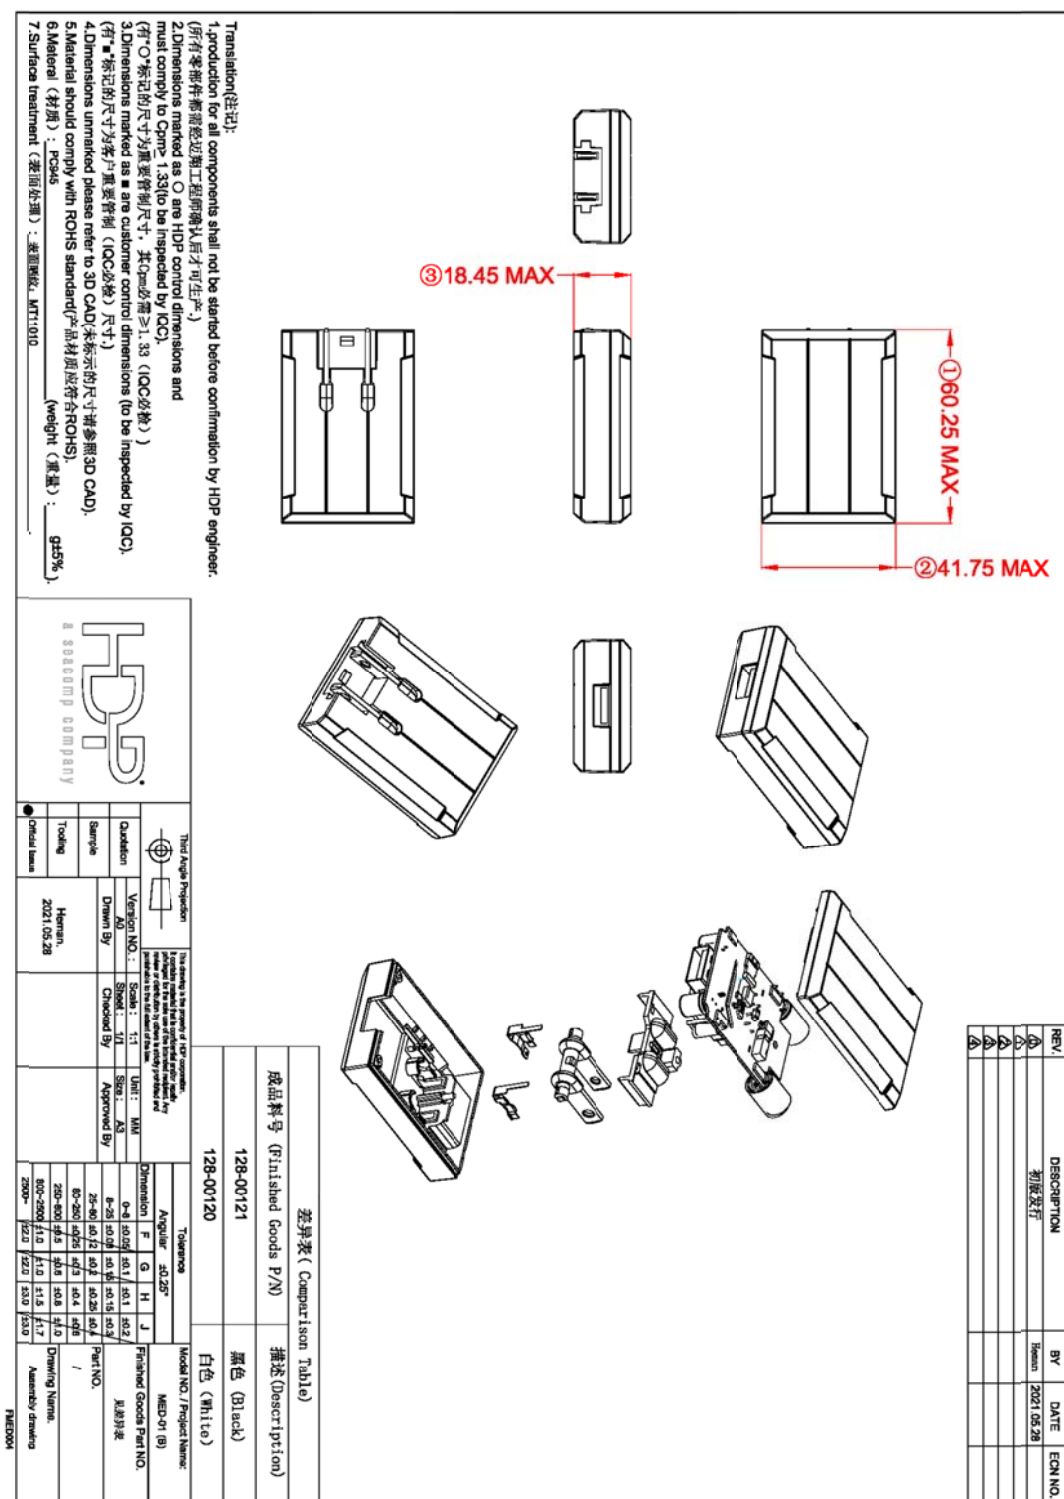


MODEL NUMBER	HDP05-MD05010U	PAGE	14 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

UK Adapter

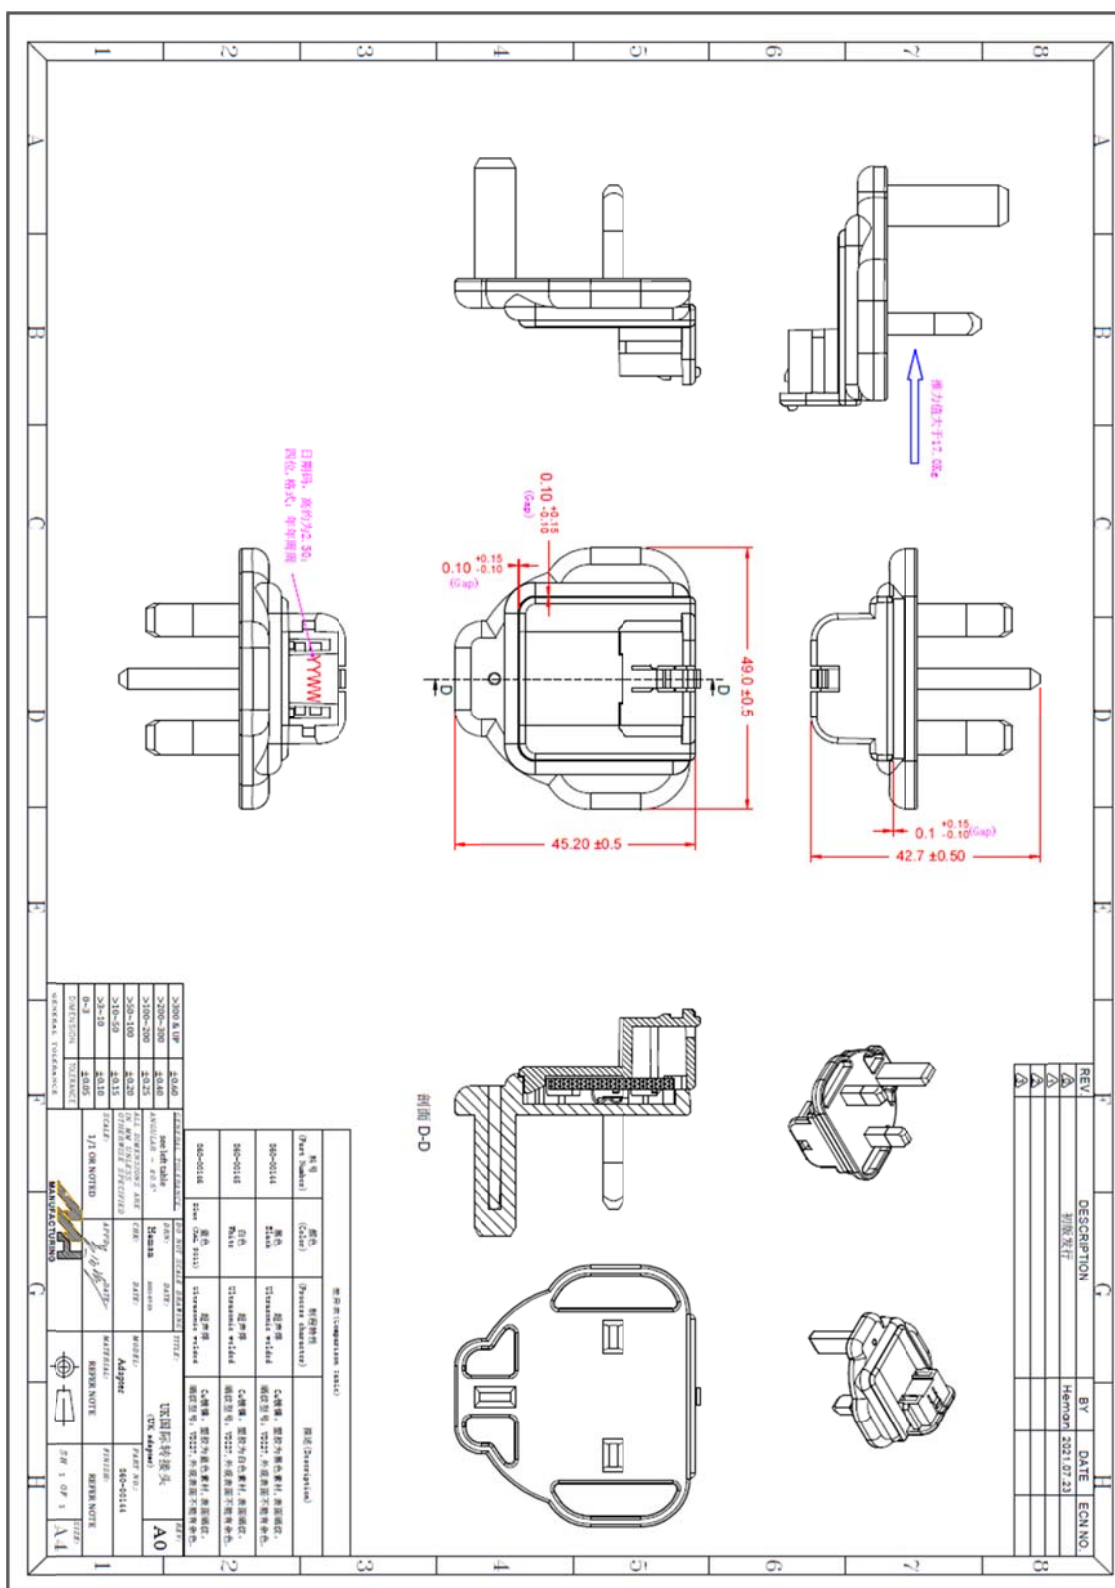


MODEL NUMBER	HDP05-MD05010U	PAGE	15 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

EU Adapter

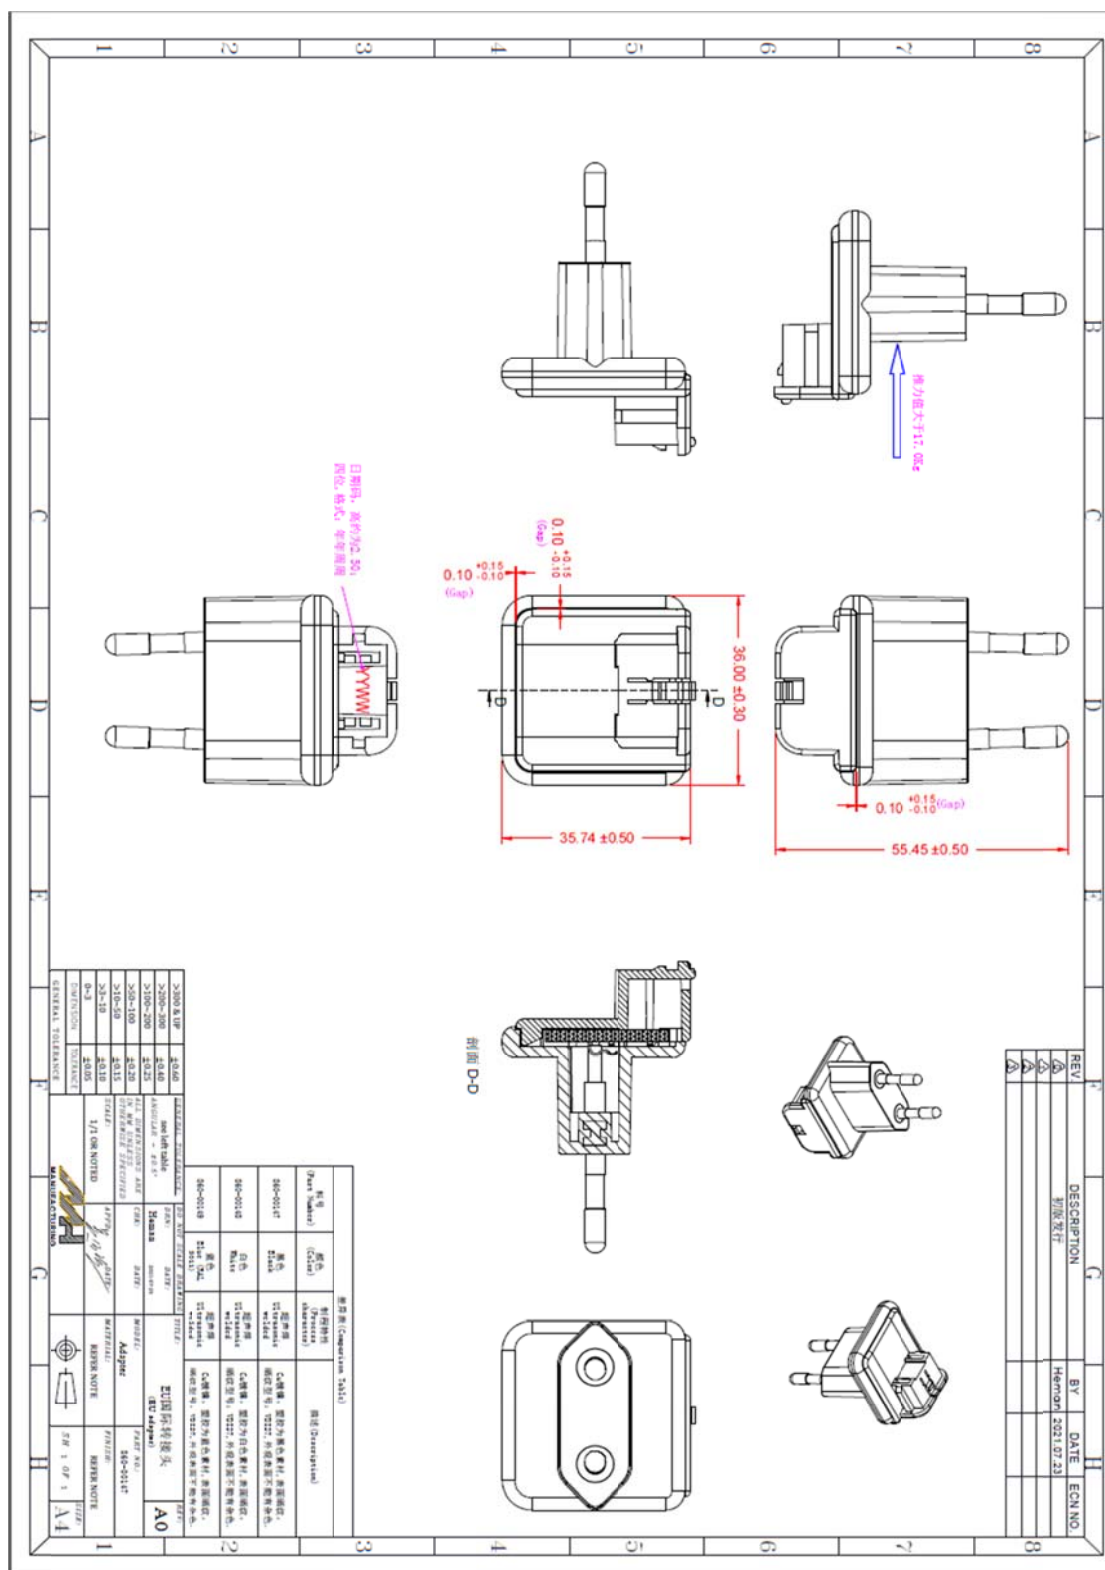

MODEL NUMBER	HDP05-MD05010U	PAGE	16 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

AU Adapter

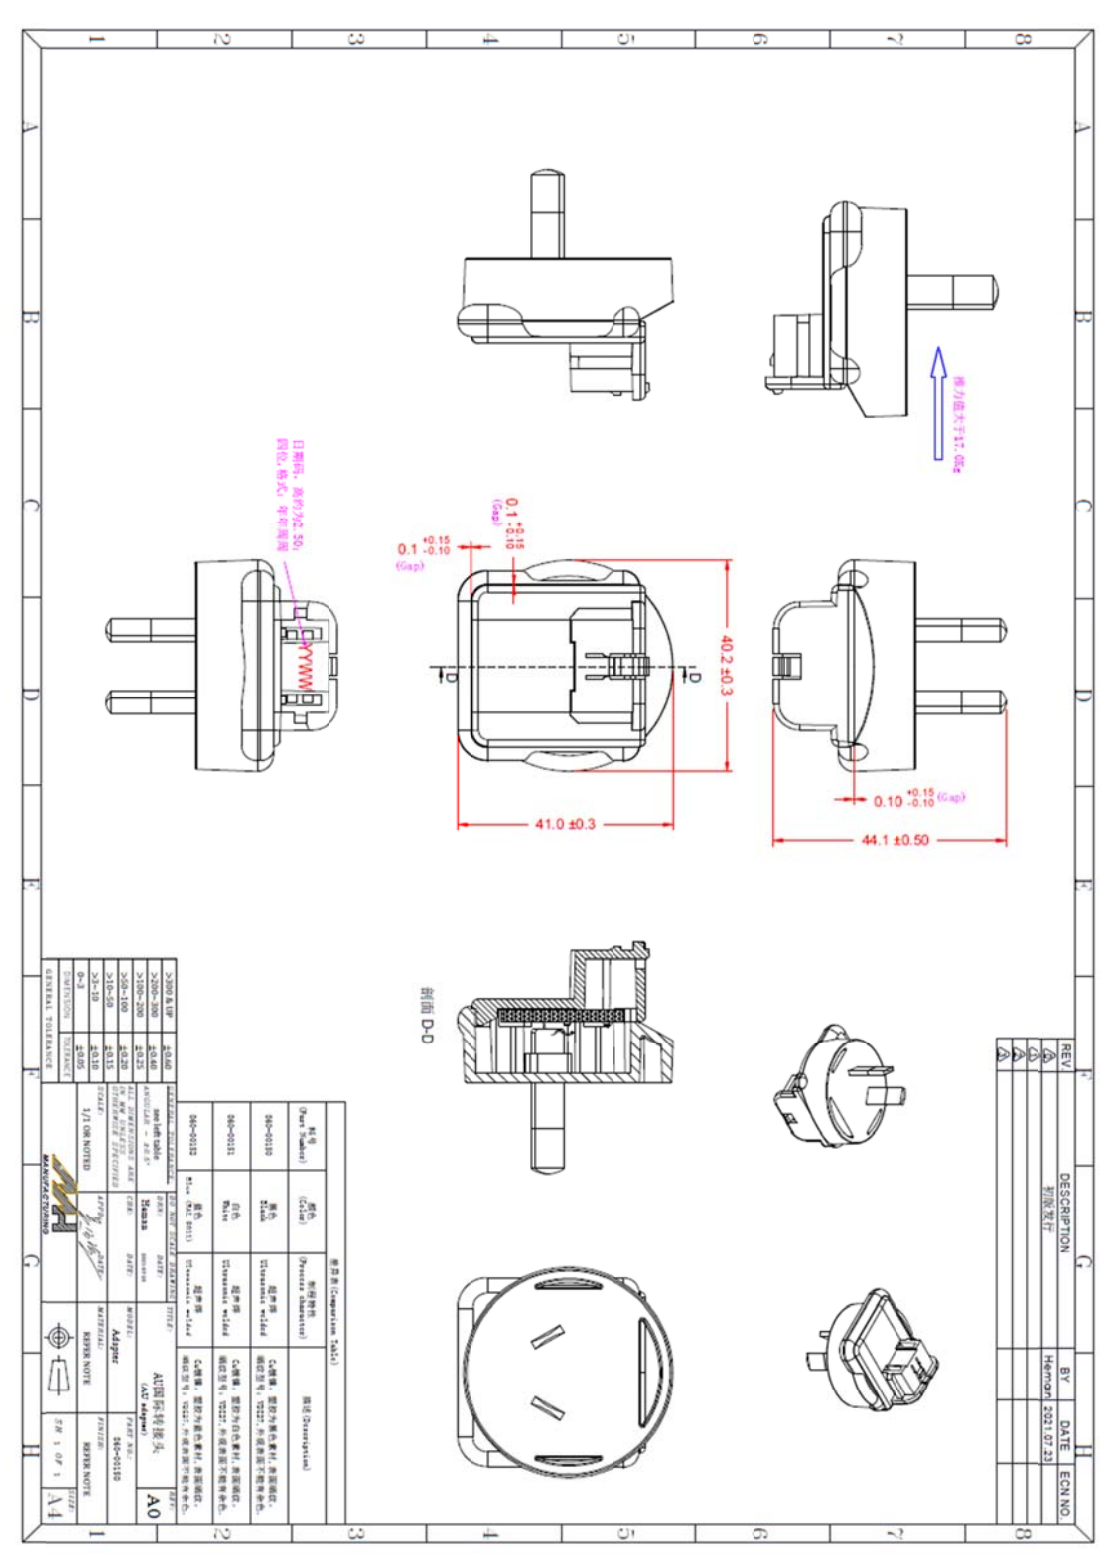

MODEL NUMBER	HDP05-MD05010U	PAGE	17 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

5 Electromagnetic Compatibility

The following tests are required:

Power Conversion Device	EU Reference	Title of Standard	International Reference	Test Level for Heavy Industrial	Test Level for Light Industrial	Test Level for 48 VDC p/s
AC-DC, DC-DC, Power Supplies	EN55032: 2015	Information technology equipment – Radio disturbance characteristics – Limits and methods of measurement	CISPR22:1997	Class "B" 4dB of margin Class "A" or Class "B" for servers	Class "B" 4dB of margin Class "A" or Class "B" for servers	Class "B" 4dB of margin Class "A" or Class "B" for servers
DC-DC, DC-DC Power Supplies	EN55024:1998 (EN50082-2:1995 updated to EN61000-6-2:2001 for -48 VDC supply)	Information technology equipment – Immunity Characteristics – Limits and methods of measurement	CISPR24:1997			Different tests and limits for DC power supplies
AC-DC, AC-DC Power Supplies	EN61000-3-2:2000 (PFC Power Supplies ONLY if rated greater than 75W)	Electromagnetic Compatibility (EMC) – Part 3: Limits – Section 2: Limits for harmonic current emissions (Equipment input current up to and including 16 A per phase)	IEC 61000-3-2:2000	Must meet Class D requirements	Must meet Class D requirements	N/A
AC-DC, AC-DC Power Supplies	EN61000-3-3:1995 (PFC Power Supplies ONLY)	Electromagnetic Compatibility (EMC) – Part 3: Limits – Section 3: Limitation of voltage fluctuations and flicker in low-voltage supply systems for equipment with rated current up to and including 16A	IEC 61000-3-3:1994	Meet specification	Meet specification	N/A
AC-DC, DC-DC, Power Supplies	EN61000-4-2	Electromagnetic Compatibility (EMC) – Part 4: – Section 2: Electrostatic discharge immunity test	IEC 1000-4-2	(+/-) 2, 4, 8, 12 and 15 kV air (+/-) 2, 4, 6, 8 kV contact discharge	(+/-) 2, 4, 8, 12 and 15 kV air (+/-) 2, 4, 6, 8 kV contact discharge	(+/-) 2, 4, 8, 12 and 15 kV air (+/-) 2, 4, 6, 8 kV contact discharge
AC-DC, DC-DC, Power Supplies	EN 61000-4-3 + Israeli Deviations in SI 961 part 6.2	Electromagnetic Compatibility (EMC) – Part 4: – Section 3: Radiated, radio-frequency electromagnetic field, immunity test	IEC 1000-4-3 Basic Standard ENV 50140	10V/m 80-1000MHz, 80% AM 900 +/- 5MHz 50%, 200Hz	3V/m 80-1000MHz, 80% AM 900 +/- 5MHz 50%, 200Hz	10V/m 80-1000MHz, 80% AM 900 +/- 5MHz 50%, 200Hz
AC-DC, DC-DC, Power Supplies	EN 61000-4-4	Electromagnetic Compatibility (EMC) – Part 4: – Section 4: Electrical fast transient/burst immunity test	IEC 1000-4-4	1, 2, 4kV – Power 0.5, 1, and 2kV – Signal	1, 2 kV – Power 0.5, 1 kV – Signal	1, 2 kV – Power 0.5, 1, and 2kV – Signal
AC-DC, DC-DC, Power Supplies	EN 61000-4-5	Electromagnetic Compatibility (EMC) – Part 4: – Section 5: Surge Immunity Test	IEC 1000-4-5	1, 2kV differential 2, 4kV common	0.5, 1 kV diff. 0.5, 1, 2, 2.5 common	0.5, 1kV differential 0.5 1kV common
AC-DC, DC-DC, Power Supplies	EN 61000-4-6 + Israeli Deviations in SI 961 part 6.2	Electromagnetic Compatibility (EMC) – Part 4: – Section 6: Conducted disturbances induced by radio-frequency fields – immunity test	IEC 1000-4-6 Basic Standard ENV 50141	10V/m 80% AM (1kHz)	3 V/m 80% AM (1kHz)	10 V/m 80% AM (1kHz)
AC-DC, DC-DC, Power Supplies	EN 61000-4-8	Electromagnetic Compatibility (EMC) – Part 4: – Section 8: Power-frequency magnetic field immunity test	IEC 1000-4-8	30 A/m (r.m.s.)	1 A/m (r.m.s.)	30 A/m (r.m.s.)
AC-DC, DC-DC, Power Supplies	EN 61000-4-11	Electromagnetic Compatibility (EMC) – Part 4: – Section 11: Voltage dips, short interruptions and voltage variations immunity test	IEC 1000-4-11	30% for 0.5 S >95% for 10mS >95% for 5 S	30% for 0.5 S >95% for 10mS >95% for 5 S	30% for 0.5 S >95% for 10mS >95% for 5 S

Light Industrial: EN55022:1998 (Emission) and EN 61000-6-1:2001 (Immunity)

Heavy Industrial: EN55011 (Emission) and EN 610006-2:2005 (Immunity)

The content of the test report, at a minimum, includes:

- Test object used (development status with serial number/sample name)
- Mode(s) of operation of the test object
- Test result
- Photograph/sketch of the test environment along with listed test conditions
- Applied measurement tools/equipment
- Ambient temperature for ESD-tests. Also include air pressure and air humidity
- Name of Test Engineer
- Date of the test

MODEL NUMBER	HDP05-MD05010U	PAGE	18 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

6 Labeling


6.1 Labeling the Device

The labeling must comply with IEC 60950 , IEC62368 and IEC 60601 requirements.

The following information as a minimum must be printed on the adapter:

- Input rating
- Output rating
- Made in China
- Model and/or part number
- Production lot or date code

6.2 Label Drawing

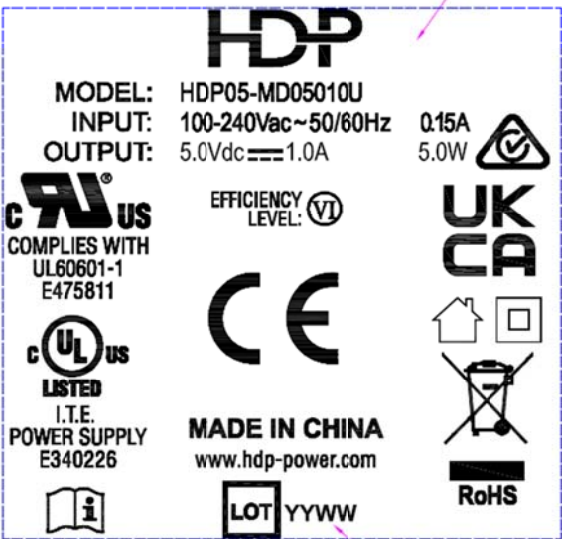


Laser print on this mark
此部分字樣用鐳雕

底殼放大圖

此處內容為鐳射 "YYWW"

REV.	DESCRIPTION	BY	DATE	ECN NO.
△	初版發行	Reman	2022.03.05	
△				
△				
△				
△				

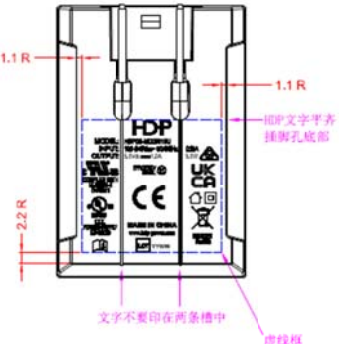

Laser Printing of this bottom mark
底面字樣鐳光標繪

印中文字字樣
鐳射孔底部

文字不要印在兩條槽中

虛線框
不要印上去

注意事項:
X.X R = Reference dimension


料 号		描述	
HDP05-MD-0004		白色 / White	
HDP05-MD-0005		黑色 / Black	

Third Angle Projection		Tolerance		Model NO. / Project Name:	
Quantity	Version NO.:	Scale: 1:1	Unit: MM	HDP05-MD05010U	
Sample	Drawn By	Sheet: 1/1	Size: A1	Finished Goods Part NO., MED01 5V 1A USB	
Tooling	Checked By	Checked By	Approved By	Part NO. See Note	
Official Issue	Reman.	2022.03.05		Drawing Name, Laser Printing drawing	
				FME000	

MODEL NUMBER	HDP05-MD05010U	PAGE	19 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

7 Packaging

7.1 Drawing

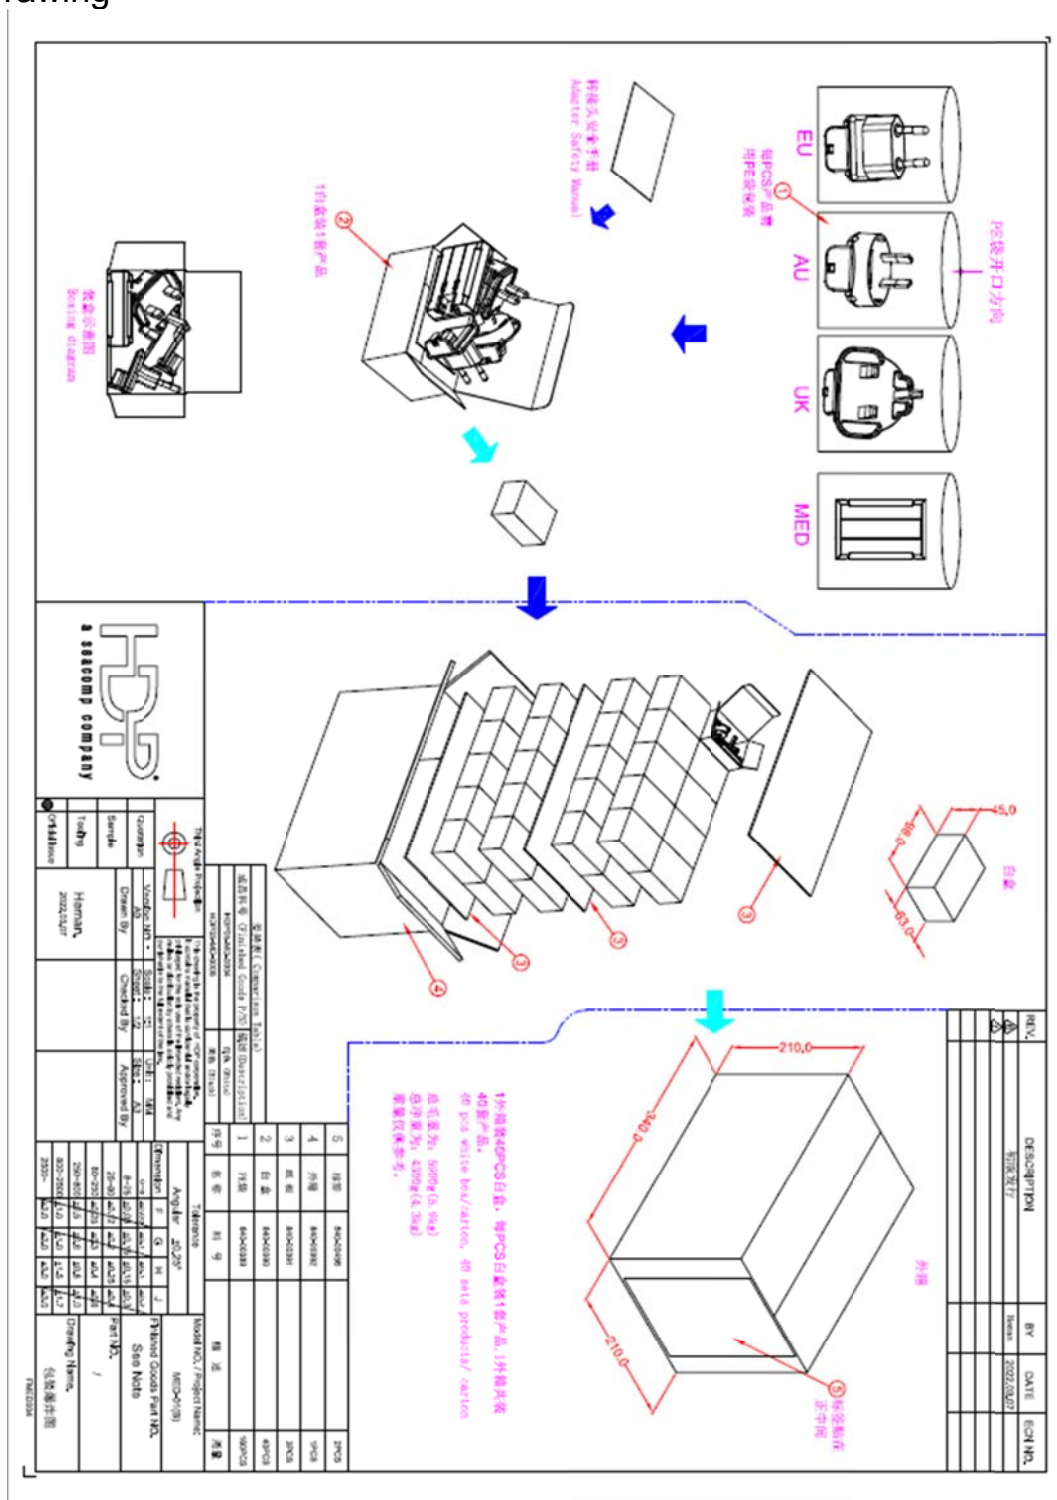

MODEL NUMBER	HDP05-MD05010U	PAGE	20 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

Master Carton Label

210.00

148.00

Front Height:
Around 5.3mm

Front Height:
Around 4.3mm

SEACOMP

PN: XXXXXXXXXXXX

QTY: XXX PCS

P/O NO: XXXXXXXX

DATE CODE: XXXXXXXX

GROSS WEIGHT: XX.XX KG

NET WEIGHT: XX.XX KG

SIZE: XX x XX x XX CM

CARTON: X/X

SEACOMP

261 GATEWAY ROAD, CAULSBAD,
CALIFORNIA 92008 USA

TEL: 714-244-0000

FAX: 714-244-0001

EMAIL: SALES@SEACOMP.COM

MADE IN CHINA

Print the label (Self-made)

打印标签(自制)

Font: Arial

A5 Blank Label (Purchasing)

A5 空白标签/ 材质: 白底铜版纸 (采购)

P/N: 840-00456



SEACOMP

THE ARTIST'S SIGNATURE		THE ARTIST'S SIGNATURE	
Signature	Date	Signature	Date
Handwritten Signature	2022.03.07	Handwritten Signature	2022.03.07

SEACOMP

261 GATEWAY ROAD, CAULSBAD,
CALIFORNIA 92008 USA

TEL: 714-244-0000

FAX: 714-244-0001

EMAIL: SALES@SEACOMP.COM

MADE IN CHINA

THE ARTIST'S SIGNATURE		THE ARTIST'S SIGNATURE	
Signature	Date	Signature	Date
Handwritten Signature	2022.03.07	Handwritten Signature	2022.03.07

MODEL NUMBER	HDP05-MD05010U	PAGE	21 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

Safety Manual

Translation/注意:

1. production for all components shall not be started before confirmation by HDP engineer.
(所有零件都需经过工程确认后才可以生产.)

2. Dimensions marked as $\varnothing$ are HDP control dimensions and must comply to Cpk: 1.33 to be inspected by IQC.
(待“ $\varnothing$ ”标记的尺寸为重要管制尺寸, 其Cpk必需 ≥ 1.33 (IQC必检))

3. Dimensions marked as $\blacksquare$ are customer control dimensions (to be inspected by IQC), (待“ $\blacksquare$ ”标记的尺寸为客户重要管制 (IQC必检) 尺寸)

4. Dimensions unmarked please refer to 3D CAD.未标示的尺寸请参考3D CAD.

5. Material should comply with ROHS standard.产品材质应符合ROHS.

6. Material (材料): $\varnothing$ weight (重量): $\geq 15\%$.

7. Surface treatment (表面处理): $\varnothing$

SEACOMP

COMPANY INFORMATION

HDP Power - a SEACOMP company
2545 Gateway Road
Campbell, CA, USA 92009

TELEPHONE: +1760 918 6722
EMAIL: info@seacomp.com
WEBSITE: www.seacomp.com

FIRST EDITION • FEBRUARY 2022

HDP

POWER

a SEACOMP COMPANY

Note:

1. 双面印刷, 白底蓝字;
2. 板框号: 80;板框尺寸:
3. 对折尺寸:
4. 内容排版须参照以下源文件一致:
840-00380_Adapter-Safety-Manual-EN-DE1.pdf

Safety Information

① 100x310 (对折前宽度)

② 80x310

对折后背面 (对折前宽度)

对折后正面

内页左侧

SAFETY NOTES FOR MAINS ADAPTERS

- Only use the mains adapter in indoor areas. Never use it in wet rooms or in the rain.
- Keep the mains adapter, its electrical parts and its accessories away from children.
- Only connect the mains adapter if the mains voltage of the socket corresponds to the voltage of the mains adapter.
- Only connect the mains adapter to an easily accessible socket so that you can quickly disconnect it from the mains.
- Do not expose the mains adapter to extreme temperatures, direct sunlight, intense moisture, flammable vapours, or chemicals.
- Never touch the mains adapter with damp or wet hands. Otherwise there is a risk of electric shock.
- The product will heat up during operation. Do not cover the mains adapter with objects and do not place it on a flammable surface.
- If the mains adapter is moved from a cold environment to a warm one, condensation may form, which could damage the electronic components. Wait until the condensation has dried up before using the adapter.
- Do not modify the mains adapter.
- Keep the mains adapter away from open fire and hot surfaces.

内页右侧

SICHERHEITSHINWEISE FÜR NETZTEILE

- Verwenden Sie das Netzteill nur in Innenräumen. Verwenden Sie es nie im Regen, in Bädern oder an anderen feuchten Stellen.
- Halten Sie das Netzteill, seine elektrischen Teile und seine Zubehörteile von Kindern fern.
- Schließen Sie das Netzteill nur an, wenn die Netzspannung der Steckdose mit der Angabe auf dem Netzteill übereinstimmt.
- Schließen Sie das Netzteill nur an eine gut zugängliche Steckdose an, damit Sie das Netzteill schnell vom Stromnetz trennen können.
- Setzen Sie das Netzteill keinen extremen Temperaturen, direktem Sonnenlicht, Feuchtigkeit, feuchter Luft, brennbaren Dämpfen oder chemischen Substanzen aus.
- Berühren Sie das Netzteill niemals mit nassen oder feuchten Händen.
- Das Produkt erwärmt sich während des Betriebs. Bedecken Sie das Produkt nicht mit Gegenständen und stellen Sie es nicht auf brennbare Oberflächen.
- Wenn das Netzteill von einer kalten Umgebung in eine warme Umgebung gebracht wird, kann Kondensation entstehen, die die elektronischen Bauteile beschädigen kann. Warten Sie, bis die Kondensation vollständig getrocknet ist, bevor Sie das Netzteill verwenden.
- Verändern oder modifizieren Sie das Netzteill nicht. Sie das Netzteill von offener Flamme und heißen Flächen fern.

Table 1: Dimensions

Dimension	F	G	H	J
Overall width	100	100	100	100
Overall height	310	310	310	310
Overall depth	310	310	310	310
Overall weight	150	150	150	150

Table 2: Material Properties

Property	Value
Material	PC
Color	Black
Surface treatment	Electrocoat
RoHS compliance	Yes

MODEL NUMBER	HDP05-MD05010U	PAGE	22 of 22
PART NUMBER	HDP05-MD-0004	REVISION	A0
DESCRIPTION	I.T.E. & MEDICAL POWER SUPPLY BLACK , USB , with EU AU UK Adapter	DATE	Mar 11, 2022

7.2 Packaging Test

1	Bulk product	Drop package on each side for a total of 10 drops (2 opposite corners, 3 adjacent sides of bottom corner, then all 6 faces) per system on concrete floor from a height of 1.0 meter. This is an operational test. Pass/Fail Criteria: 1.The systems shall pass Functional Test. 2. No visible damage to product and gift box.
2	Drop test for Packaged Product (gift box, clamshell, etc.)	Drop fully packaged products (in gift box or clamshell) onto a concrete floor from height of 153cm for 10 drops on the six surfaces and four corners. Pass/Fail Criteria:☐ 1. The systems shall pass Functional Test. 2. Paper or PET deformation is acceptable. No damage in product integrity of packaging materials (e.g. sealed edge openings) is allowed.
3	Sinusoidal Vibration	Test with sine wave that will sweep the frequency from 7 - 500 hertz for construction test; 5 - 70 hertz for packaging test. Displacement >3.15mm. Total test duration time shall be 30 min (10 min per axis). Test shall be performed in three mutually perpendicular axes: Z-axis (vertical), Y-axis (fore-aft), and X-axis (lateral). Pass/Fail Criteria:☐ The UUT and packaging shall withstand the above test procedure without visible damage or performance decline during operation.

8 Warranty

One year warranty for defects arising from workmanship and materials per the SEACOMP Warranty, RMA, and Failure Analysis Policy.

Mouser Electronics

Authorized Distributor

Click to View Pricing, Inventory, Delivery & Lifecycle Information:

[HDP Power:](#)

[HDP05-MD-0005](#)